

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.**





## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification <sup>6</sup> : <b>A61M 5/00</b>	<b>A2</b>	(11) International Publication Number: <b>WO 95/05207</b>  (43) International Publication Date: <b>23 February 1995 (23.02.95)</b>
<p>(21) International Application Number: <b>PCT/US94/09399</b></p> <p>(22) International Filing Date: <b>18 August 1994 (18.08.94)</b></p> <p>(30) Priority Data: <b>08/109,131</b>      <b>19 August 1993 (19.08.93)</b>      <b>US</b></p> <p>(71) Applicant: <b>ENDOVASCULAR TECHNOLOGIES, INC.</b> <b>[US/US]; 1360 O'Brien Drive, Menlo Park, CA 94025 (US).</b></p> <p>(72) Inventors: <b>QUIACHON, Dinah, B.; 1872 Luby Drive, San Jose, CA 95133 (US). STERMAN, Wesley, D.; 2121 Sacramento Street #604, San Francisco, CA 94109 (US). WILLIAMS, Ronald, G.; 1313 Sherman Avenue, Menlo Park, CA 94025 (US). DILLOW, David, C.; 22851 Longdown Road, Cupertino, CA 95041 (US). BAKER, Steve, G.; 743 San Ramon, Sunnyvale, CA 94086 (US).</b></p> <p>(74) Agent: <b>THOMPSON, Clifton, W.; Fulwider, Patton, Lee &amp; Utecht, 10th floor, 10877 Wilshire Boulevard, Los Angeles, CA 90024 (US).</b></p>	<p>(81) Designated States: <b>AU, CA, JP, European patent (AT, BE, CH, DE, DK, ES, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).</b></p> <p><b>Published</b> <i>Without international search report and to be republished upon receipt of that report.</i></p>	
<p>(54) Title: <b>DUAL VALVE REINFORCED SHEATH AND METHOD</b></p> <p>(57) Abstract</p> <p>A large-diameter expandable sheath for use in introducing a catheter or other medical instrument into a vessel in the body of a patient. The expandable sheath comprises an elongate sheath tube formed of a flexible material which has proximal and distal extremities and a passage extending therethrough of a maximum predetermined diameter. The distal extremity of the elongate sheath tube is folded longitudinally to a smaller folded diameter. The sheath tube may be self-expanding or may be reinforced with a self-expanding wire or expandable stents. A backflow adapter is secured to the proximal extremity of the elongate sheath tube. The backflow adapter has a central opening therein in registration with the passage in the sheath tube. A normally closed primary valve is disposed in the central opening of the backflow adapter and is movable to an open position. A normally open secondary valve, movable to a closed position, may be configured in the backflow adapter proximal the sheath tube and distal the primary valve. The primary and secondary valves when open permit a catheter or other medical instrument to be inserted into the sheath, and when closed form a hemostatic seal about the catheter. A sheath introducer is provided for guiding the distal end of the sheath tube into a vessel and is configured to be positioned within the backflow adapter.</p>		

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	GB	United Kingdom	MR	Mauritania
AU	Australia	GE	Georgia	MW	Malawi
BB	Barbados	GN	Guinea	NE	Niger
BE	Belgium	GR	Greece	NL	Netherlands
BF	Burkina Faso	HU	Hungary	NO	Norway
BG	Bulgaria	IE	Ireland	NZ	New Zealand
BJ	Benin	IT	Italy	PL	Poland
BR	Brazil	JP	Japan	PT	Portugal
BY	Belarus	KE	Kenya	RO	Romania
CA	Canada	KG	Kyrgyzstan	RU	Russian Federation
CF	Central African Republic	KP	Democratic People's Republic of Korea	SD	Sudan
CG	Congo	KR	Republic of Korea	SE	Sweden
CH	Switzerland	KZ	Kazakhstan	SI	Slovenia
CI	Côte d'Ivoire	LI	Liechtenstein	SK	Slovakia
CM	Cameroon	LK	Sri Lanka	SN	Senegal
CN	China	LU	Luxembourg	TD	Chad
CS	Czechoslovakia	LV	Latvia	TG	Togo
CZ	Czech Republic	MC	Monaco	TJ	Tajikistan
DE	Germany	MD	Republic of Moldova	TT	Trinidad and Tobago
DK	Denmark	MG	Madagascar	UA	Ukraine
ES	Spain	ML	Mali	US	United States of America
FI	Finland	MN	Mongolia	UZ	Uzbekistan
FR	France			VN	Viet Nam
GA	Gabon				

- 1 -

TITLE

## DUAL VALVE REINFORCED SHEATH AND METHOD

This application is a continuation-in-part of application Ser. No. 07/807,089 filed on Dec. 13, 1991, which is hereby  
5 incorporated by reference.

BACKGROUND OF THE INVENTION

This invention relates to an expandable sheath and more particularly to a dual valve, reinforced, large-diameter expandable sheath and method of use.

10 Expandable access catheter assemblies have heretofore been provided to facilitate the placement and removal of diagnostic and therapeutic catheters through the vascular system. Such catheter assemblies included a flexible variable-diameter catheter body, a diameter control stylet and a flexible Y-hub.  
15 The flexible Y-hub incorporates an adjustable hemostasis valve and a side port in one branch and a diameter control stylet guide wire in another branch. A flexible variable diameter catheter body is secured to the flexible Y-hub and can be expanded between a collapsed position and an expanded position  
20 by the stylet guide wire. Several deficiencies have been found in such a device. For example, the adjustable hemostasis valve is incapable of accepting large catheters. The flexible variable-diameter catheter body is objectionable in that it has a tendency to reduce in diameter and hold onto large-diameter  
25 catheters when it is attempted to place the same through the catheter body. In addition, the tip of the stylet guide wire catches a large-diameter catheter which causes elongation of the catheter body and reduction in its diameter to grab and prevent further advancement of the large-diameter catheter.  
30 There is therefore a need for a new and improved large-diameter expandable sheath which will overcome these deficiencies.

SUMMARY OF THE INVENTION

The present invention comprises a sheath assembly for use in introducing a catheter or other medical instrument into a  
35 corporeal vessel. The sheath assembly includes an elongate

- 2 -

sheath tube formed of a flexible material having proximal and distal extremities and having a passage extending therethrough. The distal extremity of the sheath tube may have a reinforcing means for causing radial expansion of the distal extremity of the sheath tube to an expanded diameter.

The sheath assembly further includes a backflow adapter having a body with a central opening in fluid communication with the sheath tube. The backflow adapter includes a normally closed primary valve and may include a normally open secondary valve. When the primary and secondary valves are open they permit a medical instrument to be inserted into said sheath tube and when closed form a hemostatic seal about the instrument. The sheath assembly may further include a sheath introducer capable of being disposed in the passage of said sheath tube.

The primary valve is disposed proximal the secondary valve. The primary valve has a cylindrical member formed of a flexible material having a proximal end and a distal end configured with a bore therein in fluid communication with the passage of the sheath tube. The primary valve also has a ring gear secured to one end of the cylindrical member, a rack for driving the ring gear to cause relative rotation between the ends of the cylindrical member to cause the cylindrical member to be twisted to close the bore extending through the cylindrical member, and biasing means for urging the rack into a position wherein the cylindrical member is rotated to a closed position.

The secondary valve is secured to the proximal extremity of the sheath tube, and has a cylindrical member formed of a flexible material having a proximal end and a distal end configured with a bore therein in registration with the passage of the sheath tube. The secondary valve includes rotating means for engaging the cylindrical member for causing relative rotation between the ends of the cylindrical member to cause the cylindrical member to be twisted to close the bore extending through the cylindrical member.

In general, it is an object of the present invention to provide an expandable sheath which can be utilized with

- 3 -

large-diameter catheters and method for using the same. Another object of the invention is to provide a sheath of the above character which is folded longitudinally to a small diameter and which can be expanded greatly when a large-diameter catheter is to be passed through it. Another object of the invention is to provide a sheath of the above character which is provided with a backflow adapter which includes a tubular diaphragm that can be moved into an hourglass or iris-like configuration to create a fluid-tight barrier around any tubular device such as a large-diameter catheter passed through the backflow adapter and the tubular diaphragm. Another object of the invention is to provide a sheath of the above character in which a dilator can be utilized for expanding the sheath. Another object of the invention is to provide a sheath of the above character in which the backflow adaptor can be readily controlled.

Other features and advantages of the present invention will become apparent from the following detailed description, taken in conjunction with the accompanying drawings, which illustrate, by way of example, the principles of the invention.

#### BRIEF DESCRIPTION OF THE DRAWINGS

FIGURE 1 is a side elevational view of a large-diameter expandable sheath assembly incorporating the present invention and in which a sheath introducer is disposed in the sheath tube.

FIG. 2 is an enlarged side elevational view of the sheath introducer shown in the large-diameter expandable sheath assembly of FIG. 1.

FIG. 3 is an enlarged detail view partially in cross-section of the distal extremity of the sheath introducer shown in FIG. 2.

FIG. 4 is a cross-sectional view taken along the line 4-4 of FIG. 1.

FIG. 5 is a partial side elevational view of an alternative embodiment of an expandable sheath tube incorporating the present invention.

FIG. 6 is a cross-sectional view taken along the line 6-6

- 4 -

of FIG. 5.

FIG. 7 is a cross-sectional view similar to FIG. 4 showing the sheath of FIGS. 5 and 6.

5 FIG. 8 is an enlarged side elevational view partially in cross-section of the proximal extremity of the large expandable sheath of the sheath assembly shown in FIG. 1 and particularly showing the backflow adapter.

10 FIG. 9 is an end elevational view looking along the line 9-9 of FIG. 8 with certain portions being shown in cross-section and with the valve carried by the backflow adapter being in a normally closed position.

FIG. 10 is a view similar to FIG. 9, but showing the valve in an open position.

15 FIG. 11 is a side elevational view partially in cross section opposite the side shown in FIG. 8 of the proximal extremity of the expandable sheath.

FIG. 12 is a bottom plan view looking along the line 12-12 of FIG. 11.

20 FIG. 13 is a top plan view looking along the line 13-13 of FIG. 11.

FIG. 14 is a side elevational view of the valve or diaphragm utilized in the backflow adapter shown in FIGS. 9 and 10.

25 FIG. 15 is an alternative embodiment of a valve or diaphragm for use in the backflow adapter shown in FIGS. 9 and 10.

FIG. 16 is still another embodiment of a valve or diaphragm for use in the backflow adapter shown in FIGS. 9 and 10.

30 FIG. 17 is a view similar to FIG. 9 but showing an alternative rack and pinion arrangement for the backflow adapter.

FIG. 18 is a cross-sectional view showing another embodiment of a rack for the closing and opening of the valve in the backflow adapter.

35 FIG. 19 is a cross-sectional view taken along the line 19-19 of FIG. 18.

FIG. 20 is a side elevational view of an alternative embodiment of the sheath assembly incorporating the present



- 5 -

invention and in which a sheath introducer is disposed in the sheath tube.

FIG. 21 is an enlarged elevational view partially in cross-section of the proximal extremity of the sheath assembly shown in FIG. 20 and particularly showing the back-flow adapter.

FIG. 22 is a partial side elevational view of an alternative embodiment of an expandable sheath tube incorporating the present invention.

FIG. 23 is a cross-sectional view taken along the line 23-23 of FIG. 22.

FIG. 24 is an end elevational view looking along the line 24-24 of FIG. 21 with certain portions being shown in cross-section and with the primary valve being in a normally closed position.

FIG. 25 is a side elevational view partly in cross-section of the primary valve shown in FIG. 24 in an open position and held by a keeper.

FIG. 26 is an enlarged detailed view partially in cross-section of an alternate embodiment of the distal extremity of the sheath tube and the sheath introducer, showing the radiopaque marker band on the introducer and a radiopaque marker on the sheath tube.

FIG. 27 is a partial side elevational view in cross-section of an alternate embodiment of an expandable sheath tube incorporating a self-expanding reinforcement means.

FIG. 28 is a partial side elevational view of an alternate embodiment of an expandable sheath tube incorporating a helical coil.

FIG. 29 is a partial side elevational view in cross-section of an alternate embodiment of an expandable sheath tube incorporating a helical coil embedded between an inner sheath tube and an outer sheath tube.

FIG. 30 is a partial side elevational view in cross-section of an alternate embodiment of an expandable sheath tube incorporating stents and a balloon for expanding the stents.

FIG. 31 is a partial side elevational view of an alternate embodiment of an expandable sheath tube incorporating U-shaped

- 6 -

expandable wires.

FIG. 32 is a partial side elevational view of an alternate embodiment of an expandable sheath tube incorporating a wire having a circular distal end.

5        FIG. 33 is a partial side elevational view of an alternate embodiment of an expandable sheath tube incorporating an expandable wire including two half-circles at the distal end of the sheath tube.

10       FIG. 34 is a partial side elevational view of an alternate embodiment of an expandable sheath tube incorporating expandable wires forming a "W" pattern at the distal end of the sheath tube.

15       FIG. 35 is a side elevational view of a sheath assembly inserted into a vessel, wherein an introducer capsule is being removed from the sheath tube.

FIG. 36 is a side elevational view of a sheath assembly inserted in a vessel wherein a removable capsule is being used to withdraw the sheath tube from the vessel.

#### DESCRIPTION OF THE PREFERRED EMBODIMENTS

20       In general, the large-diameter expandable sheath is used for introduction of a catheter into the body of a patient. It comprises an elongate sheath tube formed of a flexible material and having proximal and distal extremities and having passage therein of a predetermined maximum diameter. The distal  
25       extremity of the elongate sheath tube is folded longitudinally into a smaller diameter. A backflow adapter is secured to the proximal extremity of the elongate sheath tube. The backflow adapter has a central opening therein in registration with the passage in the sheath tube. Valve means is disposed in the  
30       central opening in the backflow adapter and is movable between open and closed positions. The valve means when in an open position permits a catheter to be introduced into the sheath and when closed forms a liquid-tight seal about the catheter extending therethrough.

35       More particularly as shown in FIG. 1 of the drawings, the large-diameter expandable sheath 11 consists of an elongate sheath tube 12 having proximal and distal extremities 13 and 14

- 7 -

and having a flow passage 16 having a maximum diameter extending therethrough. The expandable sheath 11 can have a suitable length as, for example, fifteen to thirty-five centimeters and preferably approximately eighteen centimeters with a maximum outside diameter of one centimeter. The elongate sheath tube is formed of a flexible material having a wall thickness of 0.001 to 0.020 inches (0.0254-0.51 millimeters) and preferably about 0.005 inches (0.127 millimeters) and can be formed of a suitable plastic material such as "TEFLON" (a fluorinated ethylene propylene). An alternate material is "TEFZEL" (ethylene tetrafluoroethylene). The selected material should have physical characteristics which will not be compromised by radiation sterilization.

As shown in FIG. 4, the distal extremity of the sheath tube is pleated or folded longitudinally to provide wraps or folds 17 for a distance of approximately ten centimeters from the distal end to provide a distal extremity of reduced diameter as, for example, a reduction of the outside diameter from 3/8 to 3/16 of an inch (9.52-4.76 millimeters) or approximately one-half the original size. The folding or pleating of the sheath tube 12 in this manner serves two purposes. The first purpose is to reduce the sheath diameter to facilitate introduction of the sheath and to make it less traumatic for the vessel into which it is introduced. The second reason is that with a small-diameter, thin-wall tube, as represented by the elongate sheath tube 12, there is less likelihood of kinking occurring than in a large-diameter, thin-wall tube. The distal extremity of the sheath tube 12, when folded longitudinally in this manner, serves to provide kink resistance in the distal extremity 14 while still being relatively flexible.

If it is desired to further decrease the likelihood of kinking in the large-diameter, thin-wall tube which forms the sheath tube 12, another embodiment of the sheath tube can be provided of the type shown in FIGS. 5, 6 and 7. The sheath tube 18 shown in those figures is provided with a plurality of circumferentially spaced apart flexible elongate elements 19 which are embedded in the wall of the tube 18 and extend

- 8 -

longitudinally along the length thereof as shown in FIG. 5. The proximal extremities are offset or staggered as shown in FIG. 5 with alternate elements 19 being shorter. This offset relationship provides a gradation in stiffness in the proximal extremity of the sheath tube 18. The elongate elements 19 can be in the form of stainless steel wires having a diameter ranging from 0.005 to 0.015 inches (0.127-0.381 millimeters) and preferably a diameter of approximately 0.010 inches (0.254 millimeters). As can be seen from FIG. 6, the sheath tube 18 can bulge outwardly around the elongate elements 19 while being relatively thin between the elongate elements to retain the flexibility of the tube 18. As also can be seen from FIG. 6, the elongate elements 19 are spaced apart in the three groups to facilitate the formation of six folds 20 as shown in FIG. 7. Thus, by way of example, each set of elongate elements can have the elongate elements spaced approximately 35° apart with each set being spaced approximately 85° apart. Spacing of the elongate elements 19 in this manner facilitates the formation of the folds shown in FIG. 7. The elongate elements 19 also provide additional rigidity longitudinally of the tube 18 so as to inhibit accordioneing of the tube 18 during removal of the introducer as hereinafter described.

As shown in FIG. 22, sheath tube 12 may be provided with a sheath marker 180 located at the distal end 14 of the sheath tube. The sheath marker is formed of a radiopaque alloy, for example platinum-tungsten or platinum-iridium. The sheath marker is molded inside the distal extremity of the sheath tube to enable the physician to locate the sheath tip during the operative procedure. A laminating patch is created from a tab of sheath material located at the distal tip of the sheath. This tab is folded back over and fused to the sheath tip to laminate the radio opaque marker on the inside tip of the sheath tube. Thus, the marker resides between two laminated layers of the sheath tube. As shown in FIG. 23, the distal end of the sheath tube may be folded into four bifolds 181 to form a square-like configuration, wherein the sheath marker is embedded within one of the sides 182 of the folded square.

A backflow adapter 21 is secured to the proximal extremity

- 9 -

of the elongate sheath tube 12. The backflow adapter 21 consists of a housing or body 22 which is formed of a suitable material, for example, a plastic such as polycarbonate. The housing 22 is provided with a central bore 23 extending therethrough in axial alignment with the passage 16 of the sheath tube 12. A cylindrical sheath tube adapter 26 is disposed in the bore 23 and is provided with an annular recess 27 which receives an inwardly-extending flange 28 provided on the proximal extremity 13 of the sheath tube 12 (see FIG. 8).

10 A tubular insert 29 formed of the same material as the sheath tube 12 but of a greater wall thickness, as for example twice the wall thickness of the sheath tube 12, is secured within an annular recess 30 in the sheath tube adapter 26 by suitable means such as an adhesive. The insert 29 serves as a

15 reinforcement and serves to prevent collapse of the proximal extremities 13 of the sheath tube 12 when the expandable sheath 11 is used. The sheath tube adapter 26 is fixed within a first cylindrical collar 31 seated within the bore 23 and is held in place by solvent bonding the cylindrical collar 31 into the

20 housing or body 22 to prevent longitudinal and/or rotational movement of the first collar 31 relative to the housing or body 22. A second collar 34 is also seated in the bore 23 and is rotatable therein. An annular ring gear 36 having teeth 36 thereon is also rotatably mounted in the bore 23 as hereinafter

25 described.

A cylindrical or tubular valve member or diaphragm 40 is disposed between the first and second collars 31 and 34, and is provided with a bore or flow passage 41 extending therethrough. The valve member 40 is provided with inwardly extending annular

30 lips or flanges 42 and 43 provided on opposite extremities of the same (see FIGS. 8 and 14). The flange 43 is seated in an annular recess 46 in the sheath tube adapter 26 and is retained therein by the first collar 31. The flange 42 is seated in an annular recess 47 provided in a retaining ring 48 and retained

35 therein by the second collar 34. An annular protrusion 49 is formed integral with the retaining ring 48 and engages one side of the toothed ring gear 37 which is secured to the retaining ring 48 by suitable means such as an adhesive. Similarly, the

- 10 -

retaining ring 48 functionally engages the second collar 34 and causes the second collar 34 to rotate therewith.

The diaphragm or valve member 40 can have a suitable size as, for example, a length of 0.3 to 0.45 inches (7.62-11.43 millimeters) and preferably a length of approximately 0.3 inches (7.62 millimeters), and an inside diameter of 0.35 to 0.5 inches (8.89-12.7 millimeters), and preferably an inside diameter of 0.375 inches (9.52 millimeters), with a wall thickness ranging from 0.005 to 0.015 inches (0.127-0.381 millimeters), and preferably a wall thickness of 0.007 inches (0.178 millimeters). The annular lips 42 and 43 can extend inwardly for a distance of 0.032 inches (0.813 millimeters) from the outer wall surface and have a length of approximately 0.050 inches (1.27 millimeters). The diaphragm or valve member 40 can be formed of a suitable material, such as a silicone elastomer, as, for example, Dow "SILASTIC" 97-4720. It can have a Shore A hardness ranging from 20-80 and preferably a Shore hardness of 40A. Alternatively, a low durometer, tear-resistant rubber-like latex material can be utilized.

Other diaphragm or valve members such as shown in FIGS. 15 and 16 can be utilized which have the same physical conformation. In the embodiment shown in FIG. 15, small diener polyester fibers 52 are bonded to the exterior surface of the diaphragm 51 with a silicone adhesive so that the fibers 52 extend circumferentially around the outside surface of the diaphragm 51. Such fibers serve to impede radial and longitudinal distention of the diaphragm or valve member 51. The diaphragm or valve member 56 shown in FIG. 16 is provided with a cylindrical wall 57 which increases in thickness in a direction towards the distal extremity of the diaphragm. This helps the diaphragm to withstand the pressures applied to the diaphragm during use, which may cause the diaphragm to distend and leak.

Means is provided for causing relative rotation between the sheath tube adapter 26 and the retaining ring 48 for opening and closing the bore or flow passage 41 by twisting of the cylindrical valve member or diaphragm 40. This is accomplished by fixing the first collar 31 and the sheath tube

- 11 -

adapter 26 within the housing or body 22 by suitable means such as solvent bonding and causing rotation of the retaining ring 48 by the use of a rack 61. The rack 61 consists of a rod 62 formed of a suitable material such as stainless steel which extends through a hole 63 (see FIG. 11) in the housing or body 22 in a direction which is tangential of the bore 23. The rod 62 is disposed immediately adjacent a flange 64 formed in the body 22 against which the ring gear 36 rotates. The hole 63 opens into the bore 23 so that rack teeth 64 provided on the one side of the rod 62 engage the toothed ring gear 36 whereby upon reciprocatory movement of the rack 61, the ring gear 36 is rotated through an angle ranging from 180° to 360°, and preferably an angle of at least 270°.

An actuator 66 formed of a suitable material such as plastic is mounted on the upper extremity of the rod 62 and is secured thereto by suitable means such as an Allen-head screw 67 set into the rod 62, as shown in FIG. 13. The actuator 66 is generally rectangular in plan and is provided with an upstanding lip 68 so that it conforms to the conformation of the index finger of the hand which is to be utilized for actuating the rack 61. The actuator 66 is provided with a reinforcing rib 69 along one edge of the same. A similar actuator member 71 is provided on the body 22 underlying the actuator 66 and is also provided with a downwardly extending lip 72. The actuator member 71 is secured to the body 22 by suitable means such as an adhesive. The member 71 also has a rectangular configuration in plan and is sized so that it is adapted to be engaged by the thumb of the hand, as shown in FIG. 12. Thus, one hand can be utilized for operating the backflow adapter 21 by the index finger of the hand grasping the actuator 66 and the thumb of the same hand grasping the member 71.

A stabilization and guide rod 76 extends through a tangential bore 77 (see FIG. 11) provided in the body 22 which is spaced apart from the bore 63 and extends in a direction which is parallel thereto. The rod 76 is formed of a material such as stainless steel and is provided with a collar 78 which extends through the reinforcing rib 69 of the actuator 66 and

- 12 -

is secured therein by suitable means such as an Allen-head screw 79.

5 In an alternative embodiment of the normally closed primary valve if shown in FIGS. 24 and 25, the actuator 66 is turned 90° so that guide or stabilizer rod 76 is positioned on the opposite side of the proximal valve housing 22 to the rack 62. A ring gear 161 is configured into a gear hub 160 which causes rotation of proximal diaphragm retaining ring 158. The distal end of the primary diaphragm 40 is secured to the distal retaining ring 159 which is fixed relative to the proximal valve housing and is positioned proximal a distal retaining hub 162. The primary diaphragm is opened by depressing the actuator which causes the rack to move the ring gear and rotate the gear hub and proximal retaining ring. In addition, a cover 15 170 is added to the bottom of the body to encase the bottom portions of the rack and stabilizer rod. Also, a "C"-shaped keeper 171 can be used to maintain the actuator in the compressed or open valve position by placing one end over the actuator and the other end over bottom of the cover.

20 Referring to FIG. 11, means is provided for yieldably returning the rack 61 into a position so that the valve member or diaphragm 40 is in a normally closed position and consists of a coil spring 81 coaxially mounted on the rod 62 and having one end engaging the actuator 66 and having the other end engaging a seat 82 provided in the body 22. Means is provided for preventing the spring 81 from urging the rod 62 out of the bore 63 and consists of a lump 83 of solder or a braising material provided on the rod 62 adjacent the lower extremity of the rack teeth 64. Thus, it can be seen by the hand engaging the backflow adapter 21 using the index finger to engage the actuator 66 and the thumb to engage the actuator member 71, the rack 61 can be reciprocated back and forth to open and close a bore 86 extending through the retaining ring 48 and the sheath tube adapter 26 by forming an hourglass or iris-like closure as shown in FIG. 9 in which the radially extending lines 87 shown 35 represents the folding over of the elastomeric material of the valve member or diaphragm 40. The collar 78 provided on the stabilization rod 76 serves to stop further travel up the rack



- 13 -

when the collar 78 engage a seat 88 provided in the body 22. In this position, the spring 81 is almost completely compressed as shown in FIG. 10. Following the release of the actuator 66, the spring 81 returns the rack 62 to its home position and causes the valve member or diaphragm 40 to be completely closed as shown in FIG. 9.

The ring gear 36 can be formed of a suitable material such as stainless steel and can have any suitable number of teeth. Alternatively, the ring gear can be formed of a suitable plastic such as nylon. The other portions of the backflow adapter 21 as, for example, the body 22, the first collar 31, the second collar 34, the retaining ring 48 can be formed of a suitable plastic such as polycarbonate. The metal parts such as the rod 62, the stabilization rod 76 and the spring 81 can be formed of a suitable material such as stainless steel.

As shown in FIGS. 1 and 8, means is provided for introducing liquid as, for example, a radiopaque liquid, into the bore 86 and consists of a tube 91 formed of a suitable material such as plastic extending through the first collar 31 and through the sheath tube adapter 26 so that it is in communication with the bore 86. Flexible tubing 92 is connected to the tube 91 and has a stopcock 93 of a conventional type mounted thereon which is provided with a Luer-type fitting 94. The stopcock 93 is provided with a knob 96 which can be utilized for moving the stopcock 93 between open and closed positions.

As shown in FIGS. 20-21, an alternate embodiment of the sheath assembly 11 includes a normally open secondary valve assembly 150 located adjacent the primary valve housing 22 of the backflow adapter 21. The secondary valve assembly contains a secondary diaphragm 151 which operates substantially the same as the primary diaphragm 40 and is actuated by a thumb wheel 152. The secondary diaphragm is made of silicone and is constructed substantially the same as the primary diaphragm. The secondary diaphragm is configured to have a suitable length, diameter and wall thickness to be compatible with the primary diaphragm. Similarly, each of the materials used in the secondary valve assembly for constructing and mounting the secondary diaphragm are substantially the same as the materials

- 14 -

previously described for the backflow adapter assembly.

5 The primary valve assembly is configured similar to that described above in conjunction with FIGS. 24 and 25. Secondary valve housing 155 is provided with a central bore 165 which is  
10 in fluid communication with the central bore 23 of the primary valve housing 22 and the passage 16 of the sheath tube 12. Likewise, secondary diaphragm or valve member 151 is provided with a flow passage extending therethrough. Thus, an instrument such as the sheath introducer 101 may be passed  
15 through the primary diaphragm when the secondary diaphragm is closed, thereby preventing blood flow through the proximal end of the large-diameter expandable sheath assembly 11. Also, orifice 163 in the valve housing and orifice 164 in the sheath tube adapter 26 are provided to accept tube 91 connected to the flexible tubing 92 of a introducer sideport assembly (not shown).

As shown in FIG. 21, the secondary valve assembly 150 comprises a secondary valve housing 155 which contains secondary diaphragm 151 and thumb wheel 152. The proximal end  
20 of the secondary diaphragm is secured to the thumb wheel by proximal retaining ring 156. The distal end of the secondary diaphragm is fixed relative to the secondary valve housing by distal retaining ring 157. Rotation of the diaphragm is achieved by rotating the thumb wheel so as to cause motion to  
25 only the proximal end of the secondary diaphragm. A rotational stop (not shown) is positioned on the thumb wheel to prevent excess rotation of the secondary diaphragm. The rotational stop may be comprised of two 1/32 of an inch (0.79 millimeters) dowel pins located on the thumb wheel and the secondary valve  
30 housing which are configured to engage each other to limit the rotation of the thumb wheel. Additionally, a silicone o-ring 153 positioned proximate the thumb wheel in the primary diaphragm distal retaining hub 162 allows rotation of the thumb wheel while preventing fluid from leaking from the backflow adapter housing.  
35

A sheath introducer 101 is provided as a part of the assembly shown in FIG. 1 and as shown in FIG. 2 consists of an elongate tubular member 102 formed in three sections 103, 104

- 15 -

and 106 of different diameters. The elongate tubular member 102 can be formed of a suitable plastic material such as "PEBAX" which is formed of polyether Block Amides which is loaded with approximately 10% barium sulfate to make the same visible under X-rays. Section 103 can have a diameter ranging from 0.15 to 0.3 inches (3.81-7.62 millimeters) and preferably an outside diameter of 3/16 of an inch (4.75 millimeters). The section 104 can have a suitable diameter as, for example, 0.08 to 0.15 inches (2.03-3.81 millimeters) and preferably a diameter of 1/8 of an inch (3.17 millimeters). The section 106 can have a diameter ranging from 0.06 to 0.12 inches (1.52-3.05 millimeters) and preferably a diameter of 0.08 inches (2.03 millimeters). The distal extremities of the sections 103 and 104 are provided with tapers 107 and 108, respectively, so as to provide a tapered transition from one diameter to another. A Luer-type fitting 111 is mounted on the proximal extremity of the tubular section 103. A bore or lumen 112 (see FIG. 4) of a suitable size as, for example, one capable of passing a 0.038 inches (0.97 millimeters) guidewire, is provided in the section 106 as well as in the sections 104 and 103 extending the length of the tubular member 102.

As shown in FIG. 3, a tube 116 is mounted on the distal extremity 106 of the sheath introducer 101 and is formed of a suitable material such as silicone and is retained thereon in a suitable manner by the use of polyethylene shrink tubing 117. A cylindrical enlargement or annular bump 121 is provided on the tubular section 106 adjacent the distal extremity of the shrink tubing 117 and serves to prevent the sleeve 116 and the shrink tubing 117 from accidentally slipping off of the distal extremity of the tubular section 106.

When the sheath introducer 101 is disposed in the expandable sheath 11, as shown in FIG. 1, the proximal extremity of the silicone sleeve 116 is disposed over the distal extremity of the sheath tube 12 and serves to prevent the sharp edges of the folded sheath tube 12 from causing trauma to the interior wall of a vessel when it is introduced into the vessel when the sheath is introduced as hereinafter described. A vent hole 123 is provided in the sheath

- 16 -

introducer 101 which is in communication with the passage 112 proximal of the silicone sleeve 116, as shown in FIG. 3. The vent hole 123 can be utilized for flushing the elongate sheath tube 12 through the side port fitting 94 prior to use of the expandable sheath in a surgical procedure.

As shown in FIG. 26, a radiopaque marker band 185 may be positioned proximal to distal end of the sheath introducer 101. The marker band is made of a radiopaque alloy, platinum-tungsten or platinum-iridium. The marker band is positioned just proximal the retaining bump 121 over the elongate tubular member 102 and within silicone sleeve 116 and polyethylene shrink tubing 117. The platinum alloy band is held in place by both the silicone sleeve and the polyethylene shrink tubing. As appropriate, the marker band may be positioned elsewhere along the length of the sheath introducer, such as within the most distal tubular section 106.

Operation and use of the expandable sheath 11 in conjunction with the sheath introducer 101 may now be briefly described as follows. Let it be assumed that the patient has been prepared in a conventional manner and that it is desired to enter a peripheral vessel such as an artery or a vein of the patient. The desired vessel is exposed and a longitudinal or transverse incision made into that vessel. A guidewire of a suitable size is then selected as, for example, a guidewire having a diameter of 0.038 inches (0.97 millimeters). The guidewire (not shown) is introduced into the vessel and then the expandable sheath assembly 11 shown in FIG. 1 is placed over the guidewire by placing the proximal extremity of the guidewire into the lumen 112 provided in the elongate tubular member 102 and advanced through the Luer fitting 111. The rounded tip and the small diameter of the section 106 of the tubular member 102 facilitate advancement of the sheath introducer 101 into the vessel without traumatizing the vessel. The small-diameter tip section 106 is followed by the elongate sheath tube 12 which has been collapsed as hereinbefore described about the tubular section 106 until the sheath tube 12 has been introduced to the proper depth in the vessel. As soon as the sheath tube 12 has been positioned in the vessel,

- 17 -

the sheath introducer 101 is advanced relative to the elongate sheath tube 12 by using one hand to hold the backflow adapter 21 which is connected to the sheath tube 12 and the other hand to push the sheath introducer 101 so that the proximal  
5 extremity of the silicone sleeve 116 moves off of the distal extremity of the sheath tube 12 to expose the same.

As soon as this has been accomplished, the sheath introducer 101 is pushed forward so that section 103 enters the collapsed section of the sheath tube 12 to commence opening of  
10 the same. The sheath introducer 101 is then removed through the backflow adapter 21. The sheath introducer can be removed by grasping the backflow adapter 21 by the fingers of the hand as hereinafter described to at least partially open the same to permit removal of the sheath introducer and dilator 101 while  
15 minimizing the flow of blood from the sheath tube 12. The backflow adapter can then be released. The sheath 11 and its backflow adapter is now in its normally closed state to provide a hemostatic seal closing the flow passage 86.

The physician conducting the procedure then selects the  
20 desired catheter or other device which is desired to be introduced through the expandable sheath 11. Such a device should have a diameter of 8.5 millimeters or less or which is at least slightly less than the diameter of the bore 86. The physician grasps the actuator members 66 and 71 and presses the  
25 same to operate the rack 61 to open the diaphragm or valve member 40 permitting the physician to insert the device as, for example, the catheter through the expandable sheath 11. As soon as the catheter has been advanced as far as desired, the physician releases the pressure on the actuator members 66 and  
30 71 permitting the diaphragm 40 to close around the device as, for example, the catheter inserted through to form a hemostatic seal about the catheter. If it is desired to reposition the catheter, it is merely necessary to push or pull the catheter and it will slide freely through the diaphragm. When it is  
35 desired to remove the catheter, the catheter need only be pulled out of the sheath 101 and the diaphragm will seal closed forming a hemostatic seal.

A silicone coating may be applied to the pleated sheath

- 18 -

5 tube 12. Coating may be applied to the inner and outer surfaces prior to attachment to the backflow adapter 21. The silicone coating on the inside diameter of the sheath tube reduces the amount of force required to advance catheters and the like through the sheath tube. Additionally, the silicone coating on the outside of the sheath tube may reduce the amount of force required to advance the expandable sheath 11 into a vessel. A suitable silicone coating material is "HYDRO-SIL-D 1.0" available from TUA systems of Sarasota, Florida. 10 Additionally, a silicone lubricant may be applied to the ring gear 36 on the primary valve assembly and the adjacent to bearing surfaces.

15 The method for introducing a medical instrument into the body of a patient using the dual valve expandable sheath assembly 11 shown in FIGS. 21-26 involves opening the valves to minimize blood flow through the sheath assembly 11. First, the sheath introducer 101 is placed within the sheath assembly such that the distal end 14 of the sheath tube 12 resides in the introducer sleeve 116, as shown in FIG. 26. This step may be 20 performed as part of the manufacturing process. After the patient is prepared for the procedure, the sheath tube and the sheath introducer are intraluminally inserted into the patient, usually through a cutdown in a vessel such as a femoral artery. The distal end 106 of the sheath introducer is then inserted 25 into the vessel until the distal end of the sheath tube is within the vessel. The sheath introducer is then advanced into the vessel relative to the sheath tube, allowing the distal end of the sheath tube to expand. In addition, the sheath introducer may be further advanced into the sheath assembly to 30 dilate the distal end of the sheath tube.

Next, the sheath introducer 101 is removed from the sheath assembly 11. As the distal end 106 of the sheath introducer is removed from the sheath tube 12, the secondary valve 151 is closed to form a substantially fluid tight seal between the 35 passage 16 in the sheath tube and the secondary valve assembly 150. After the secondary diaphragm 151 is closed, the primary diaphragm 40 may be opened to fully remove the sheath introducer. Then the distal end of a catheter or other medical

- 19 -

instrument may be inserted through the primary valve. The primary diaphragm is then closed to form a substantially fluid tight seal around the medical instrument. Next, the secondary diaphragm is opened to allow the distal end of the medical instrument to be inserted through the secondary valve assembly, through the passage in the sheath tube and into the vessel of the patient. After the procedure has been completed, the medical instrument and the sheath assembly can be removed from the vessel and the incision which has been made in the vessel for permitting passage of the sheath assembly can be sutured.

It can be seen from the foregoing that there has been provided an expandable sheath 11 which can be made in various sizes to accommodate large-diameter devices while still providing the desired hemostatic seal. The expandable sheath can be readily inserted and removed. The sheath introducer 101 facilitates this introduction. It is provided with a distal extremity 106 which is small in diameter to permit the sheath tube 12 to be wrapped about the same as hereinbefore described. The sheath introducer 101 is provided with sections 103 and 104 of larger diameters to provide additional rigidity to the sheath introducer 101 to facilitate pushing of the sheath introducer when introducing the expandable sheath 11 into the vessel of the patient.

An alternative mechanism for actuating the diaphragm 40 is shown in FIG. 17 and consists of a pinion 131 which engages the ring gear 36 and is disposed in a cylindrical recess 132 provided in the body 22. The pinion 131 is mounted on a shaft 133. Another gear 134 is mounted on the shaft 133 and has a smaller diameter than the diameter of the pinion 131 and engages the rack teeth 64 provided on the rod 62. By providing such a gear arrangement, it can be seen that it is possible to provide a shorter rack to achieve the same degree of ring gear rotation for opening and closing of the diaphragm 40.

As can be seen in FIGS. 18 and 19, there is shown another embodiment of a mechanism for actuating the diaphragm 40. As shown therein it consists of a flexible rack 141 that is comprised of a flexible member 142 which is provided with rack teeth 143 on one side of the same which are adaptable to engage

- 20 -

the ring gear 36. The member 142 extends through a semi-circular slot 144 provided in the body so that it extends through the body and around the ring gear 36. An actuator 146 is provided formed integral with the rack 141 for operating the rack 141 with the fingers of the hand. In this construction the rack is substantially contained within the body 22.

As shown in FIGS. 27-36, the expandable sheath 11 may include a reinforced sheath tube 200. The reinforced sheath tube is similar to the elongate sheath tube 12 and similarly has proximal and distal extremities 201 and 202. A flow passage 203 is provided having a maximum diameter extending therethrough. One suitable material for the reinforced sheath is in an expanded PTFE (polytetrafluoroethylene). Such materials may be obtained from Impra of Temp, Arizona and W. L. Gore of Flagstaff, Arizona. An example of a suitable size for a sheath tube for use with large catheter systems would include an outer diameter of approximately 0.345 inches (8.76 millimeters) with a wall thickness of 0.005 inches (0.127 millimeters) and having a length of about twenty centimeters.

The reinforced sheath tube 200 could be supported by stents, coiled wire, coiled plastic or similar means. As shown in FIG. 27, a series of self-expanding supports 210 may be placed within the sheath tube for radial expansion. Similarly, as shown in FIG. 28, a coil 211 may be attached to the outside of the sheath tube to allow for self-expansion. Alternatively, the coil support may be embedded within an inner sheath tube 212 and outer sheath tube 213, as shown in FIG. 29. The coil or expansion system may be made of a 0.012 inches (0.3 millimeters) nitinol or similar alloy wire. As shown in FIG. 30, the reinforced sheath may include balloon expandable stents 214 which may be expanded by a balloon 215 and catheter 216 or similar means.

Alternatively, the sheath tube 200 may be made of a dacron graft 217 supported by longitudinally positioned nitinol wires 218 as shown in FIGS. 31-34. As shown in FIG. 31, the reinforcement wires may be run as tightly parallel U-shaped expansion means. Likewise, a single wire forming a circle at the distal end 202 of the sheath tube may be used. Similarly,



- 21 -

two wires forming half-circles at the distal end may be used to reinforce and expand the sheath as shown in FIG. 33. Alternatively, the wires may form a "W" shape at the distal end of the sheath tube to provide radial expansion, as shown in FIG. 34.

As shown in FIG. 35, the large-diameter expandable sheath assembly 11 includes an introducer capsule 220. The reinforced sheath tube 200 is packed into the introducer capsule for deployment. The introducer capsule has a significantly less inner diameter than the outer diameter of the expanded sheath tube. The introducer capsule is configured such that it will peel away from the proximal end 201 of the reinforced sheath tube as the introducer capsule is withdrawn from the distal end 202 of the sheath tube. As the sheath introducer capsule is withdrawn, the reinforced sheath tube expands radially within the vessel.

As shown in FIG. 36, a removal capsule 225 may be fitted around the proximal 201 end of the reinforced sheath tube 200 to collapse the expanded sheath tube after the sheath tube has been deployed in a vessel. The removal capsule is configured with a lengthwise slit so it may be fitted over the proximal end of the secondary valve without having to fit over the backflow adapter 21. The removal capsule outer diameter is less than the outer diameter of the expanded sheath tube so as to radial collapse the sheath tube to a smaller diameter state. Once the reinforced sheath tube is collapsed, the removal capsule and sheath tube are then removed from the vessel. This retrieval reduces potential vessel trauma from removing a large diameter sheath.

While several particular forms of the invention have been illustrated and described, it will be apparent that various modifications can be made without departing from the spirit and scope of the invention. For example, references to materials of construction and specific dimensions are also not intended to be limiting in any manner and other materials and dimensions could be substituted and remain within the spirit and scope of the invention. Accordingly, it is not intended that the invention be limited, except as by the appended claims.

- 22 -

CLAIMS

What is claimed is:

1. A sheath assembly comprising:

an elongate sheath tube formed of a flexible material having proximal and distal extremities and having a passage extending therethrough;

5 a first valve secured to the proximal extremity of said sheath tube and movable between open and closed positions, said first valve having a central opening therein in registration with the passage in said sheath tube; and

a second valve disposed proximal said first valve and  
10 movable between open and closed positions, said second valve having a central opening therein in registration with the central opening in said first valve and with the passage in said sheath tube,

wherein said first valve and said second valve when open  
15 permit a medical instrument to be inserted into said sheath tube and when closed form a hemostatic seal about the instrument.

2. The sheath assembly of claim 1, wherein said first valve comprises:

a first cylindrical member formed of a flexible material having a proximal end and a distal end configured with a bore  
5 therein in registration with the passage of said sheath tube; and

first rotating means for engaging the cylindrical member for causing relative rotation between the ends of the cylindrical member to cause the cylindrical member to be  
10 twisted to close the bore extending through the cylindrical member.

3. The sheath assembly of claim 2, wherein said second valve comprises:

a second cylindrical member formed of a flexible material having a proximal end and a distal end configured with a bore  
5 therein in registration with the bore of said first cylindrical member; and

- 23 -

second rotating means for engaging the second cylindrical member for causing relative rotation between the ends of the second cylindrical member to cause the second cylindrical member to be twisted to close the bore extending through the  
5 second cylindrical member.

4. The sheath assembly of claim 3, wherein the second rotating means of said second valve includes a ring gear secured to one end of the second cylindrical member, and a rack for driving the ring gear to cause rotation of the second cylindrical member.

5. The sheath assembly of claim 4, wherein the second rotating means of said second valve further comprises biasing means for urging the rack into a position wherein the second cylindrical member is rotated to a normally closed position.

6. The sheath assembly of claim 5, wherein the second rotating means of said second valve further comprises an actuator carried by the rack and configured to be engaged by the fingers of a human hand for moving the rack against the  
5 force of the biasing means to move the second valve to an open position.

7. The sheath assembly of claim 6, wherein the second rotating means of said second valve further comprises a stabilizer rod slidably mounted parallel to the rack and secured to the actuator.

8. The sheath assembly of claim 1, wherein said sheath tube includes reinforcing means for causing radial expansion of said sheath tube.

9. The sheath assembly of claim 8, wherein said reinforcing means includes a self-expanding wire.

10. The sheath assembly of claim 1, wherein the distal extremity of said sheath tube is provided with a radiopaque

- 24 -

marker.

11. The sheath assembly of claim 1, wherein said sheath tube is provided with a lubricating coating.

12. The sheath assembly of claim 2, wherein the first rotating means of said first valve is provided with a lubricating coating.

13. The sheath assembly of claim 3, wherein the second rotating means of said second valve is provided with a lubricating coating.

14. The sheath assembly of claim 1, wherein the distal extremity of said sheath tube is folded longitudinally to a smaller folded diameter.

15. The sheath assembly of claim 14, further comprising a sheath introducer capable of being disposed in the passage of said sheath tube, said sheath introducer having a distal extremity extending beyond the proximal extremity of said sheath tube and dilation means positioned at the distal extremity of the sheath introducer for unfolding the sheath tube.

16. The sheath assembly of claim 15, wherein the distal extremity of said sheath introducer is provided with a radiopaque marker.

17. A sheath assembly for use in introducing a catheter into a corporeal vessel, the sheath assembly comprising:  
an elongate sheath tube formed of a flexible material having proximal and distal extremities and having a passage extending therethrough, the distal extremity of said sheath tube having a reinforcing means for causing radial expansion of the distal extremity of said sheath tube to an expanded diameter;

a first valve secured to the proximal extremity of said

- 25 -

sheath tube, said first valve having a first cylindrical member formed of a flexible material having a proximal end and a distal end configured with a bore therein in registration with the passage of said sheath tube, and having first rotating  
5 means for engaging the cylindrical member for causing relative rotation between the ends of the cylindrical member to cause the cylindrical member to be twisted to close the bore extending through the cylindrical member; and

a second valve disposed proximal said first valve, said  
10 second valve having a second cylindrical member formed of a flexible material having a proximal end and a distal end configured with a bore therein in registration with the bore of said first cylindrical member, a ring gear secured to one end of the second cylindrical member, a rack for driving the ring  
15 gear to cause relative rotation between the ends of the second cylindrical member to cause the second cylindrical member to be twisted to close the bore extending through the second cylindrical member, and biasing means for urging the rack into a position wherein the second cylindrical member is rotated to  
20 a closed position.

18. The sheath assembly of claim 17, wherein said reinforcing means includes a self-expanding wire.

19. The sheath assembly of claim 18, wherein the self-expanding wire of said reinforcing means is configured to transverse the length of said sheath tube and to form a sinusoidal shape along the perimeter of the distal extremity of said sheath tube.

20. The sheath assembly of claim 17, further comprising a sheath introducer disposed around said sheath tube, said sheath introducer having a distal extremity which has a diameter less than the expanded diameter of said sheath tube.

21. The sheath assembly of claim 18, wherein the distal extremity of said sheath tube is provided with a radiopaque marker, and the distal extremity of said sheath introducer is

- 26 -

provided with a radiopaque marker.

22. A backflow adapter having a body with a central opening in fluid communication with a sheath tube, the backflow adapter comprising:

5 a first diaphragm disposed in the central opening of said backflow adapter, said first diaphragm having a first end and a second end and being movable between open and closed positions;

10 first retaining means for engaging said first diaphragm for causing relative rotation between the ends of said first diaphragm;

15 a second diaphragm disposed in the central opening of said backflow adapter and adjacent the second end of said first diaphragm, said second diaphragm having a first end and a second end and being movable between open and closed positions; and

second retaining means for engaging said second diaphragm for causing relative rotation between the ends of said second diaphragm.

23. The backflow adapter of claim 22, wherein said second retaining means includes a gear secured to the second diaphragm and a rack for driving the gear to cause rotation of the second diaphragm.

24. The sheath assembly of claim 23, wherein the second retaining means further comprises biasing means for urging the rack into a position wherein the second diaphragm is rotated to a closed position.

25. The sheath assembly of claim 24, wherein the second retaining means further comprises an actuator carried by the rack for moving the rack against the force of the biasing means to move the second diaphragm to an open position.

26. The sheath assembly of claim 25, wherein the second retaining means further comprises a stabilizer rod slidably

- 27 -

mounted parallel to the rack and secured to the actuator.

27. The backflow adapter of claim 22, further comprising a sheath tube adapter secured to the body of said backflow adaptor and secured to a sheath tube so as to prevent rotation of said sheath tube adapter when either said first diaphragm or  
5 said second diaphragm are rotated within the body of said backflow adapter.

28. An expandable sheath for use in introducing a medical instrument into a body, the sheath comprising:

an elongate sheath tube having proximal and distal ends having an annular passage therethrough, said elongate sheath  
5 tube having a wall of substantially uniform thickness and being formed of a flexible material; and

reinforcing means for causing radial expansion of said sheath tube.

29. The expandable sheath of claim 28, wherein said reinforcing means includes a self-expanding wire.

30. The expandable sheath of claim 29, wherein the self-expanding wire of said reinforcing means is sinusoidal in configuration.

31. The expandable sheath of claim 29, wherein the self-expanding wire of said reinforcing means is helical in configuration.

32. The expandable sheath of claim 29, wherein the self-expanding wire of said reinforcing means is configured to transverse the length of said sheath tube and to encircle the perimeter of the distal end of said sheath tube.

33. The expandable sheath of claim 29, wherein the self-expanding wire of said reinforcing means is configured to transverse the length of said sheath tube and to form a sinusoidal shape along the perimeter of the distal end of said

- 28 -

sheath tube.

34. A method for introducing a medical instrument into the body of a patient, the steps of the method comprising:

- providing an expandable sheath assembly including an elongate sheath tube with proximal and distal extremities and
- 5 having a passage extending therethrough, means for radially expanding the distal extremity of the sheath tube, a normally open first valve positioned proximate the proximal extremity of the sheath tube, a normally closed second valve positioned proximal the first valve, and a sheath introducer slidably
- 10 mounted on at least the distal extremity of the sheath tube;
- introducing the sheath tube and the sheath introducer into the body of a patient;
- removing the sheath introducer from the distal extremity of the sheath tube;
- 15 expanding the distal extremity of the sheath tube;
- closing the first valve to form a substantially fluid tight seal between the passage in the sheath tube and the second valve;
- opening the second valve;
- 20 inserting the distal end of the medical instrument through the second valve;
- closing the second valve to form a substantially fluid tight seal around the medical instrument;
- opening the first valve; and
- 25 guiding the distal end of the medical instrument through the first valve, through the passage in the sheath tube and into the body of the patient.



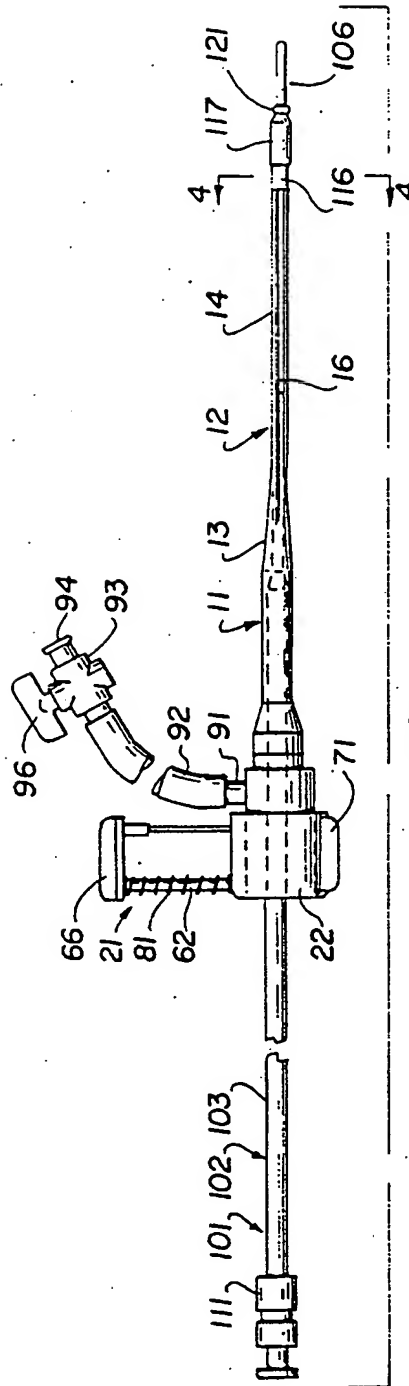


Fig. 1

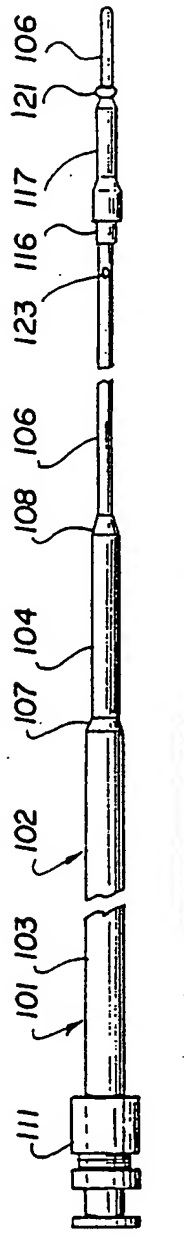


Fig. 2

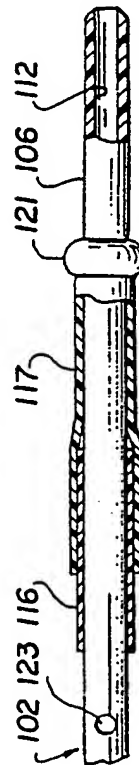


Fig. 3

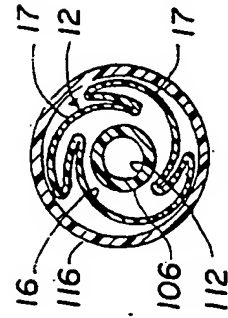
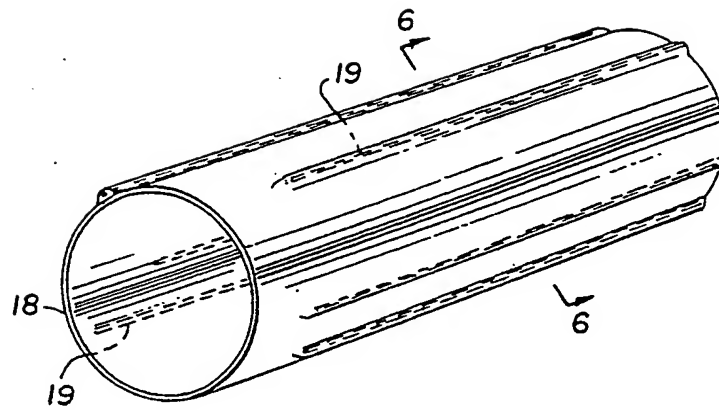
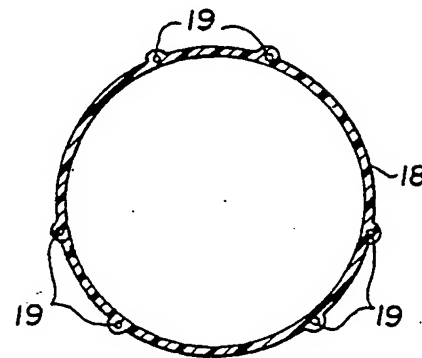
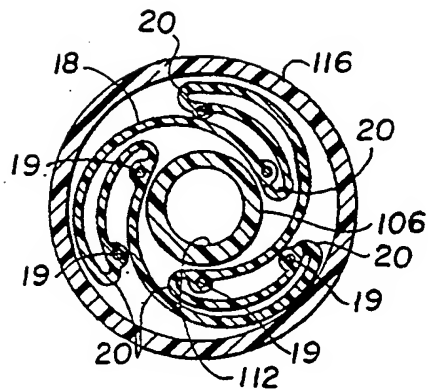


Fig. 4

*Fig.5**Fig.6**Fig.7*

3/11

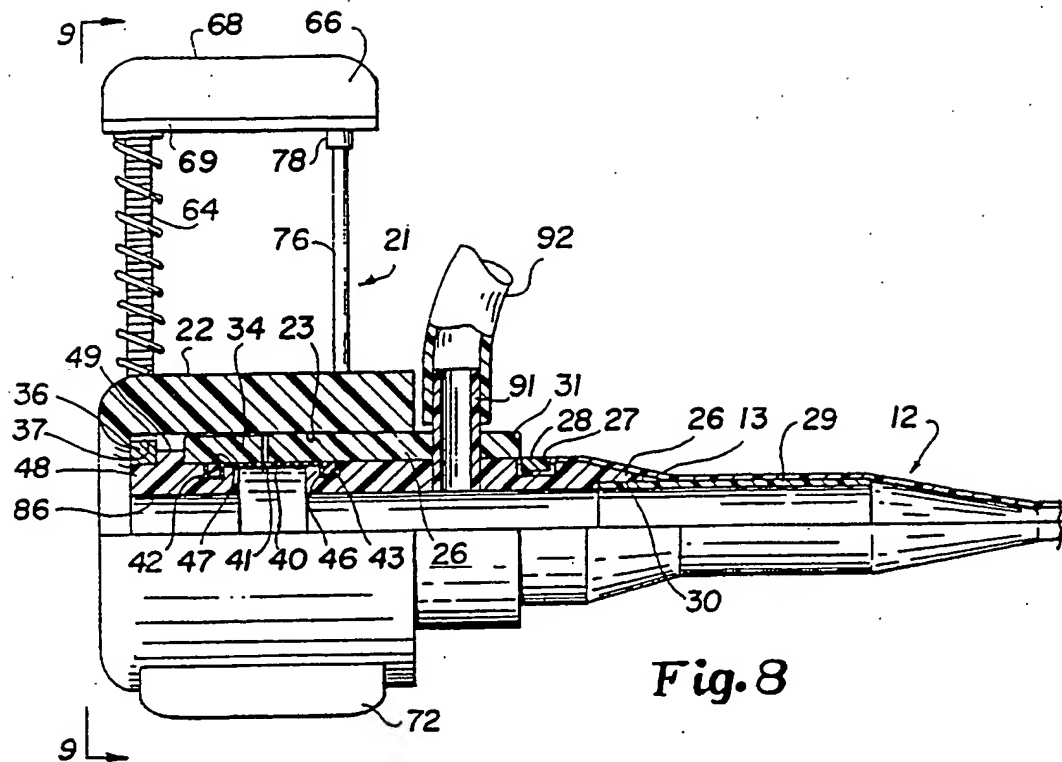


Fig. 8

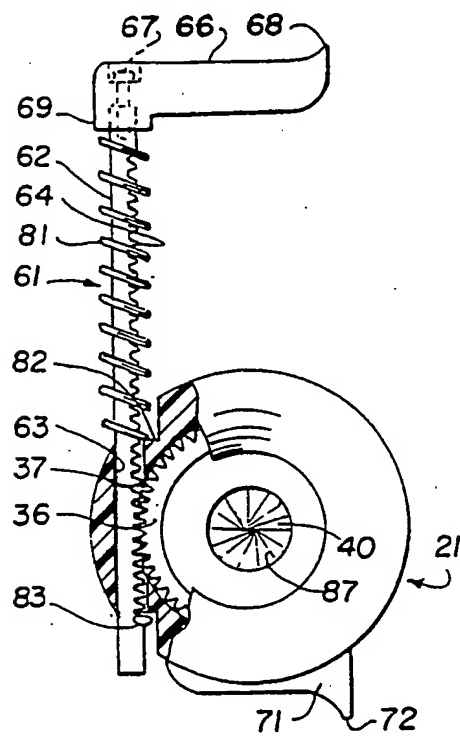


Fig. 9



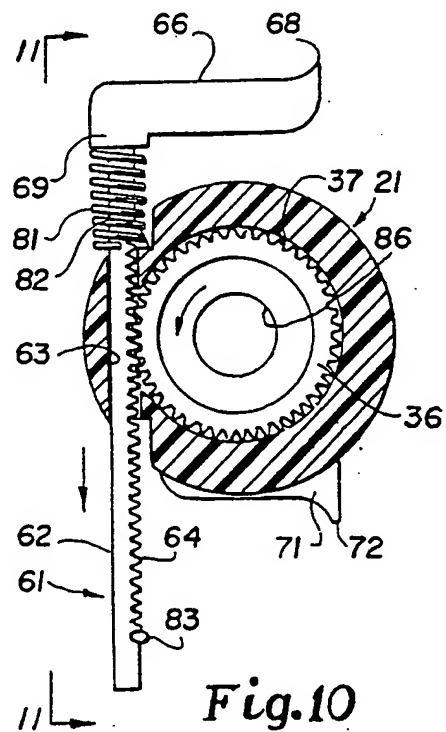



Fig. 10

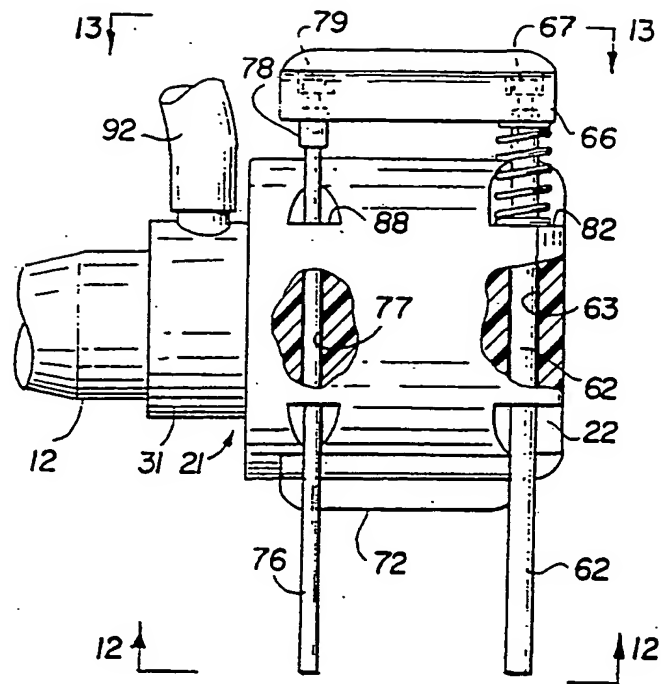

*Fig. 11*

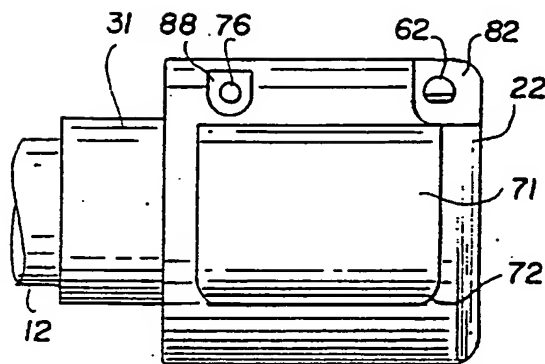

*Fig. 12*

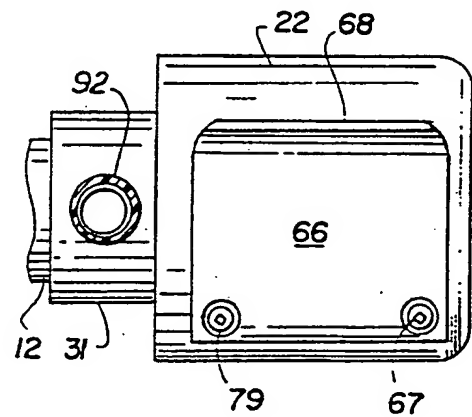

*Fig. 13*

5 / 11




Fig. 14




Fig. 15




Fig. 16

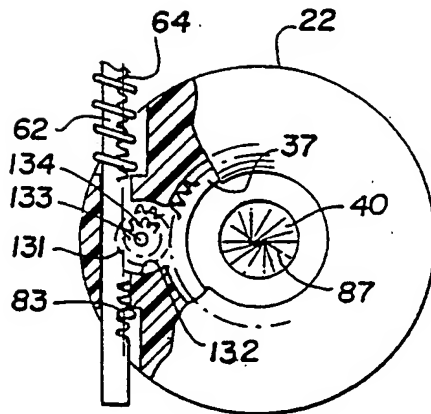


Fig. 17

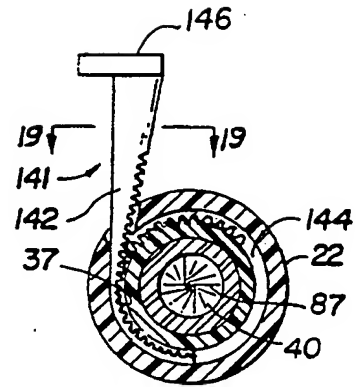


Fig. 18




Fig. 19

FIG. 20

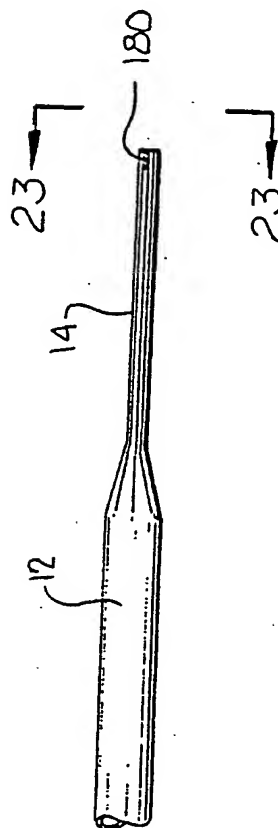
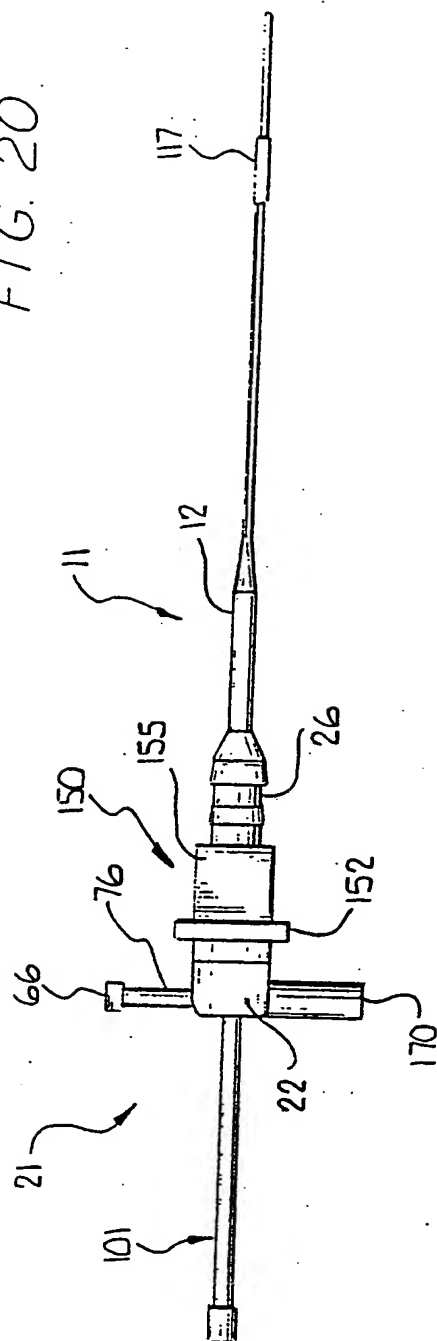


FIG. 22

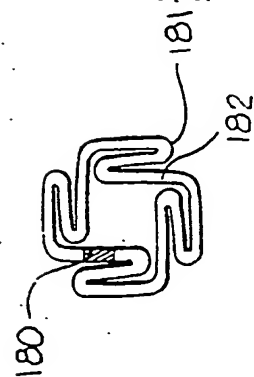


FIG. 23

7/11

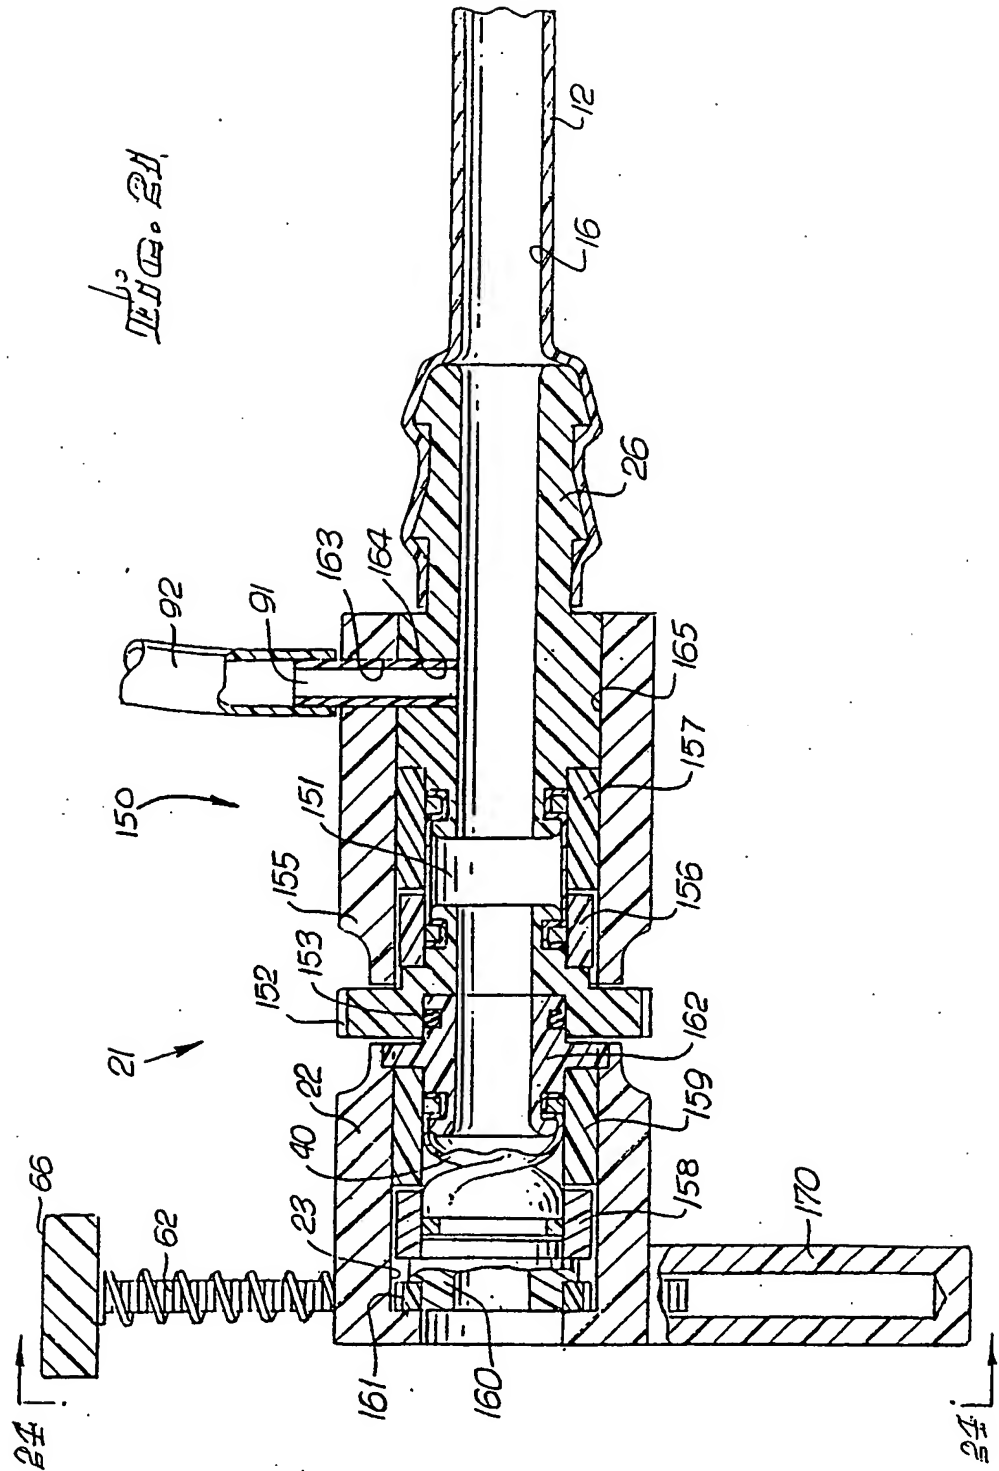


FIG. 24

8/11

FIG. 25

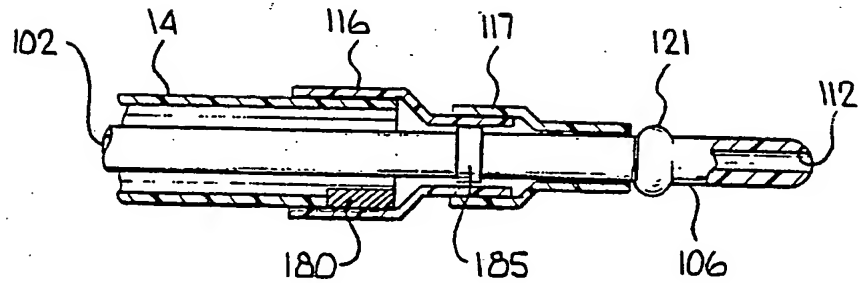
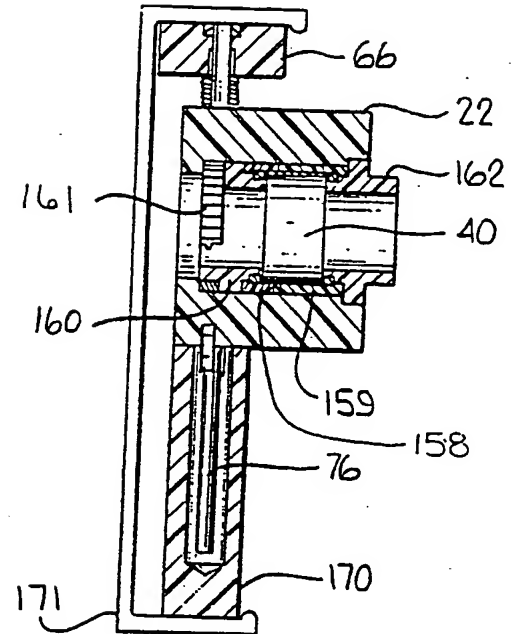
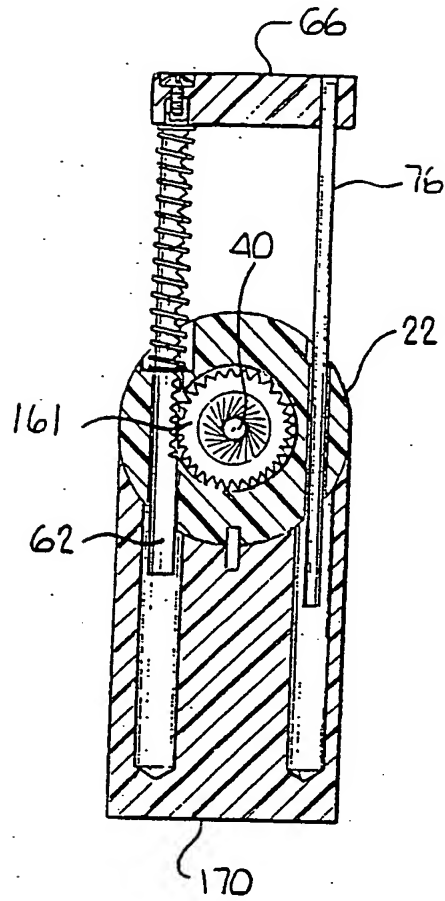


FIG. 26



FIG. 27 9/11

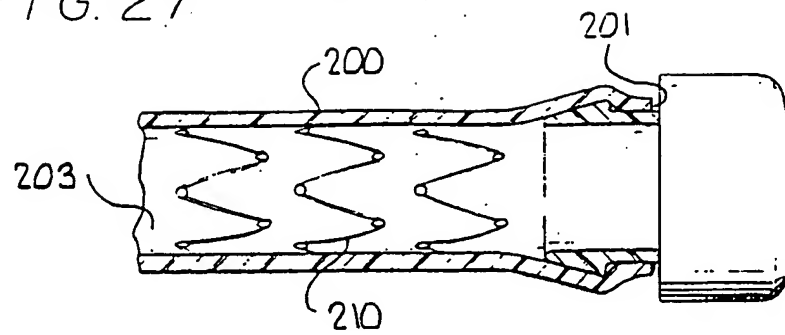


FIG. 28

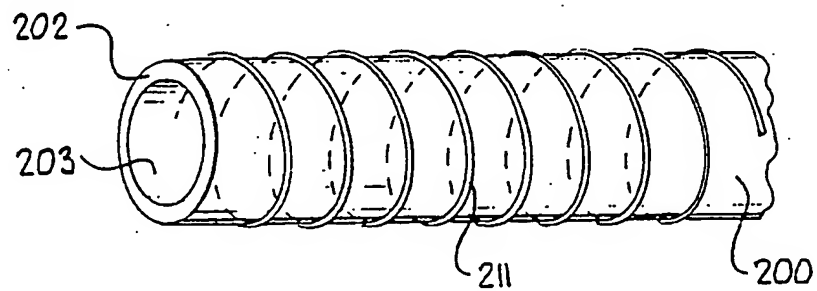


FIG. 29

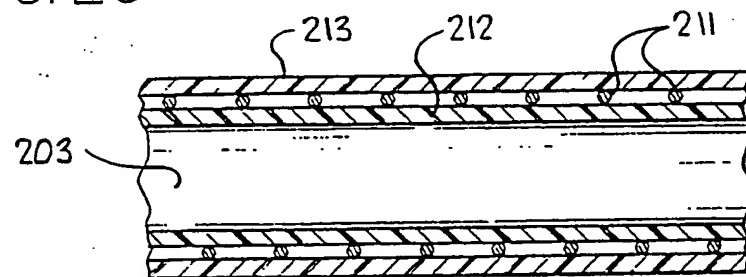


FIG. 30

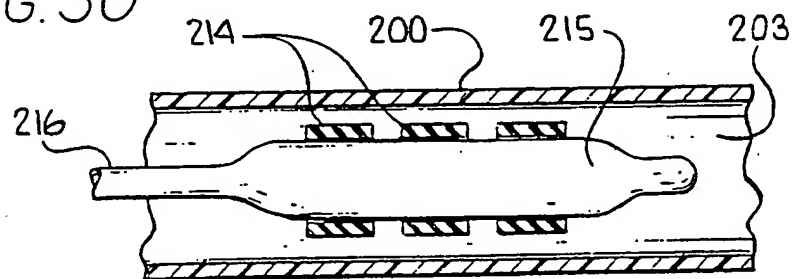


FIG. 31

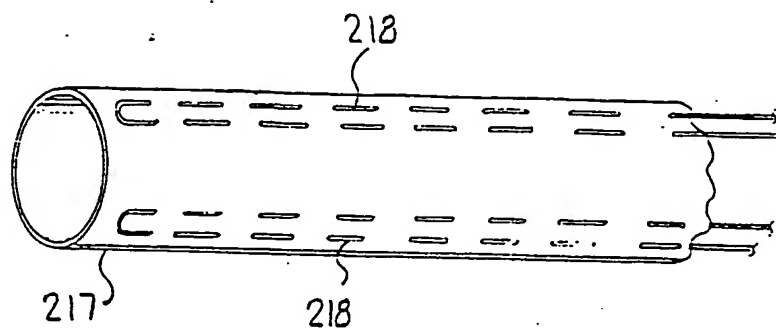


FIG. 32

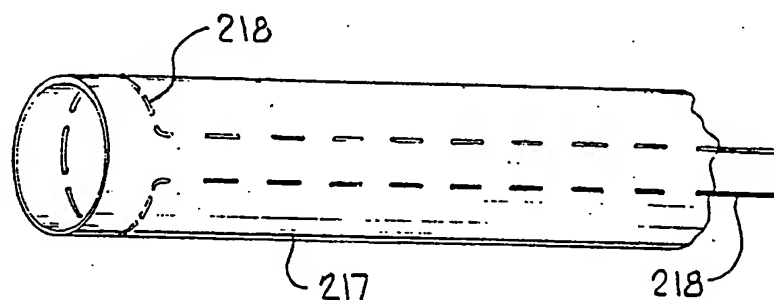


FIG. 33

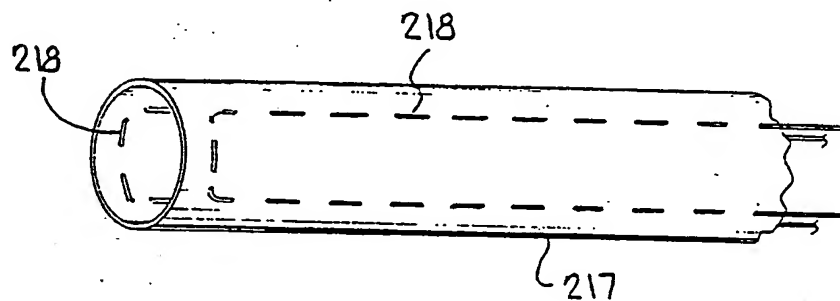
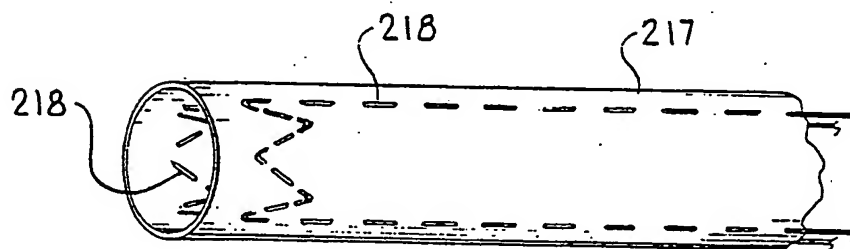


FIG. 34



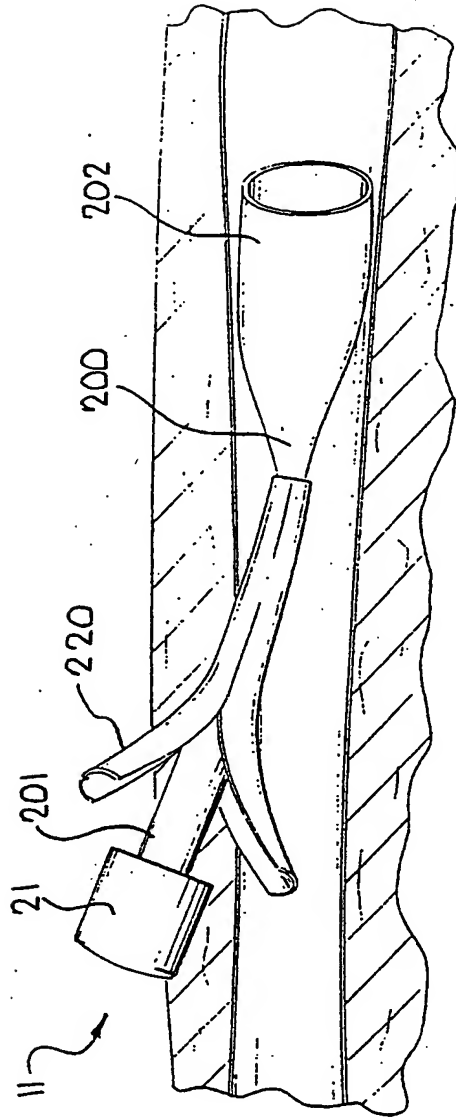


FIG. 35

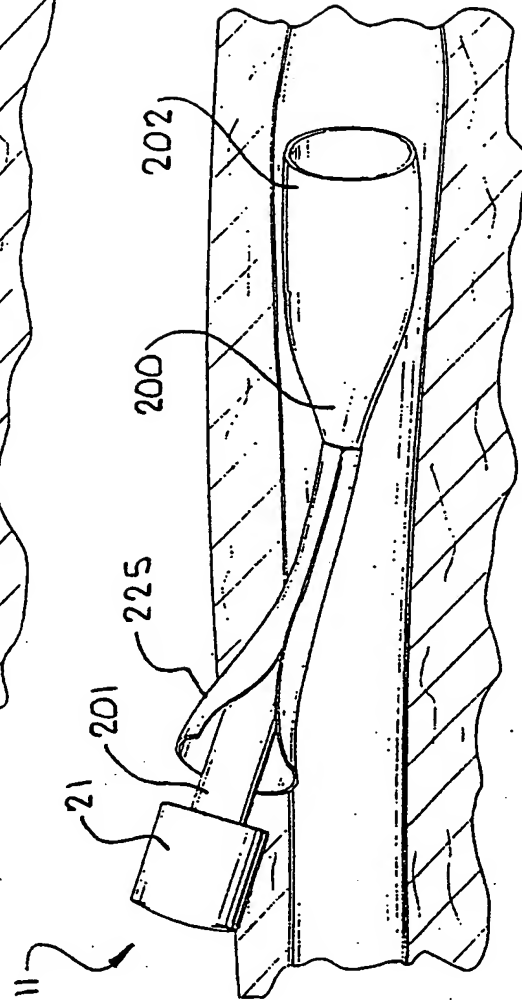



FIG. 36



## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification 6 : A61M 31/00	A3	(11) International Publication Number: WO 95/05207 (43) International Publication Date: 23 February 1995 (23.02.95)
(21) International Application Number: PCT/US94/09399 (22) International Filing Date: 18 August 1994 (18.08.94) (30) Priority Data: 08/109,131 19 August 1993 (19.08.93) US (71) Applicant: ENDOVASCULAR TECHNOLOGIES, INC. [US/US]; 1360 O'Brien Drive, Menlo Park, CA 94025 (US). (72) Inventors: QUIACHON, Dinah, B.; 1872 Luby Drive, San Jose, CA 95133 (US). STERMAN, Wesley, D.; 2121 Sacramento Street #604, San Francisco, CA 94109 (US). WILLIAMS, Ronald, G.; 1313 Sherman Avenue, Menlo Park, CA 94025 (US). DILLOW, David, C.; 22851 Longdown Road, Cupertino, CA 95041 (US). BAKER, Steve, G.; 743 San Ramon, Sunnyvale, CA 94086 (US). (74) Agent: THOMPSON, Clifton, W.; Fulwider, Patton, Lee & Utecht, 10th floor, 10877 Wilshire Boulevard, Los Angeles, CA 90024 (US).	(81) Designated States: AU, CA, JP, European patent (AT, BE, CH, DE, DK, ES, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE). Published <i>With international search report.</i> <i>Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</i> (88) Date of publication of the international search report: 27 April 1995 (27.04.95)	

(54) Title: DUAL VALVE REINFORCED SHEATH AND METHOD

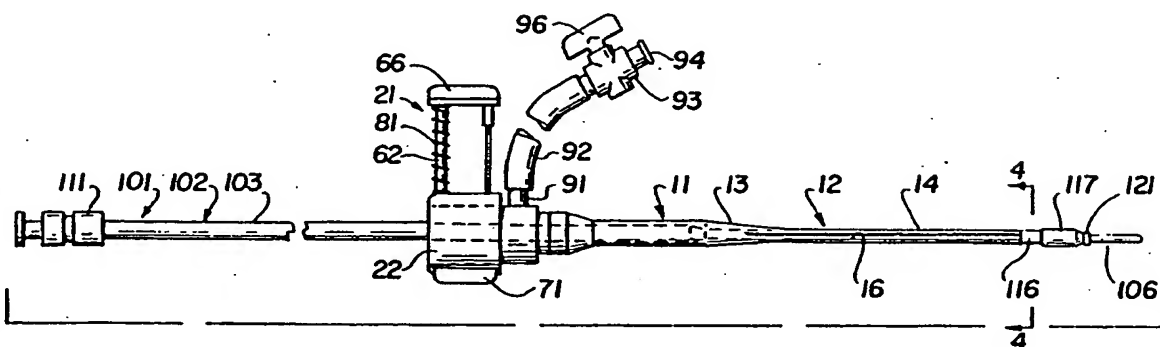

## (57) Abstract

A large diameter expandable sheath (11) for use in introducing a catheter or other medical instrument into a vessel in the body of a patient. The expandable sheath (11) comprises an elongate sheath tube (12) formed of a flexible material which has proximal (13) and distal (14) extremities and a passage (16) therethrough of a maximum predetermined diameter. The distal extremity (14) of the elongate sheath tube (12) is folded longitudinally to a smaller folded diameter. The sheath tube (12) may be self-expanding or may be reinforced with a self-expanding wire or expandable stents (19). A backflow adaptor (21) is secured to the proximal extremity (13) of the elongate sheath tube. A normally closed primary valve (40) is disposed in the central opening (23) of the backflow adaptor (21) and is movable to an open position. A normally open secondary valve (150), movable to a closed position, may be configured in the backflow adaptor (21) proximal the sheath tube (12) and distal the primary valve (40).

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	GB	United Kingdom	MR	Mauritania
AU	Australia	GE	Georgia	MW	Malawi
BB	Barbados	GN	Guinea	NE	Niger
BE	Belgium	GR	Greece	NL	Netherlands
BF	Burkina Faso	HU	Hungary	NO	Norway
BG	Bulgaria	IE	Ireland	NZ	New Zealand
BJ	Benin	IT	Italy	PL	Poland
BR	Brazil	JP	Japan	PT	Portugal
BY	Belarus	KE	Kenya	RO	Romania
CA	Canada	KG	Kyrgyzstan	RU	Russian Federation
CF	Central African Republic	KP	Democratic People's Republic of Korea	SD	Sudan
CG	Congo	KR	Republic of Korea	SE	Sweden
CH	Switzerland	KZ	Kazakhstan	SI	Slovenia
CI	Côte d'Ivoire	LI	Liechtenstein	SK	Slovakia
CM	Cameroon	LK	Sri Lanka	SN	Senegal
CN	China	LU	Luxembourg	TD	Chad
CS	Czechoslovakia	LV	Latvia	TG	Togo
CZ	Czech Republic	MC	Monaco	TJ	Tajikistan
DE	Germany	MD	Republic of Moldova	TT	Trinidad and Tobago
DK	Denmark	MG	Madagascar	UA	Ukraine
ES	Spain	ML	Mali	US	United States of America
FI	Finland	MN	Mongolia	UZ	Uzbekistan
FR	France			VN	Viet Nam
GA	Gabon				

# INTERNATIONAL SEARCH REPORT

Int. national application No.  
PCT/US94/09399

## A. CLASSIFICATION OF SUBJECT MATTER

IPC(6) :A61M 31/00

US CL :604/167, 256

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : 604/167, 256, 248, 171, 168, 169; 251/4, 345

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
	Please See Continuation of Second Sheet.	

☒ Further documents are listed in the continuation of Box C. ☐ See patent family annex.

* Special categories of cited documents:	* T	later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
* A* document defining the general state of the art which is not considered to be part of particular relevance	* X	document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
* E* earlier document published on or after the international filing date	* Y	document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
* L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	* Z	document member of the same patent family
* O* document referring to an oral disclosure, use, exhibition or other means		
* P* document published prior to the international filing date but later than the priority date claimed		

Date of the actual completion of the international search

03 MARCH 1995

Date of mailing of the international search report

30 MAR 1995

Name and mailing address of the ISA/US  
Commissioner of Patents and Trademarks  
Box PCT  
Washington, D.C. 20231

Facsimile No. (703) 305-3590

Authorized officer

PAUL HIRSCH

Telephone No. (703) 308-0858

## INTERNATIONAL SEARCH REPORT

International application No.  
PCT/US94/09399

## C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US,A, 5,158,553 (BERRY ET AL) 27 October 1992, whole document	1-2,10-12
Y	US,A, 4,540,411 (BODICKY) 10 September 1985, whole document	1-2,10-12
Y	US,A, 4,969,896 (SHORS) 13 November 1990, whole document	8-9
Y	US,A, 4,130,904 (WHALEN) 26 December 1978, whole document	8-9
Y	US,A, 5,226,913 (PINCHUK) 13 July 1993, whole document	8-9
Y	US,A, 4,850,350 (JACKSON) 25 July 1989, whole document	14-16
Y	US,A, 3,825,001 (BENNET et al) 23 July 1974, whole document	14-16
A	US,A 5,167,636 (CLEMENT) 01 December 1992, whole document	

# INTERNATIONAL SEARCH REPORT

International application No.  
PCT/US94/09399

## Box I Observations where certain claims were found unsearchable (Continuation of item 1 of first sheet)

This international report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos.:  
because they relate to subject matter not required to be searched by this Authority, namely:
2. ☐ Claims Nos.:  
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
3. ☐ Claims Nos.:  
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

## Box II Observations where unity of invention is lacking (Continuation of item 2 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

Please See Extra Sheet.

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☒ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:  
1-21,34

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest.  
☐ No protest accompanied the payment of additional search fees.



## BOX II. OBSERVATIONS WHERE UNITY OF INVENTION WAS LACKING

This ISA found multiple inventions as follows:

- I. Claims 1-21,34 drawn to a sheath assembly with resealable closure means for a conduit, classified in class 604, subclass 167.
- II. Claims 22-27 drawn to a rotative valve backflow adaptor, classified in class 604, subclass 248.
- III. Claims 28-33 drawn to a conduit sheath, classified in class 604, subclass 163.

The inventions of Groups I, II, III describe respectively a dual valve sealing assembly, a fluid control system utilizing rotative actuation, and a sheath — each of which has separate utility in either sealing about a conduit, as a sealing system independent of control and a in situ conduit or as a protective sheath (Group III).

THIS PAGE BLANK (USPTO)